



# Laser Photometer

**Model 8587A**



## **A compact, reliable photometer for customized filter testing.**

The Laser Photometer 8587A features a reliable laser diode that produces constant laser power, so aerosol concentration measurements remain stable over a long period of time. A sheath-air design keeps the optics clean for low background levels and also minimizes maintenance requirements. The 8587A utilizes an internal switching valve to measure both the upstream and downstream aerosol concentration. A special high-speed "purge" mode shortens the purge time when switching between upstream and downstream measurements.

A simple serial command set can be incorporated into your LabVIEW® or similar program to give you complete flexibility in test protocol and database management. All of these features combine to make the 8587A ideally suited for custom filter testing applications.

### **Applications**

- Respirator certification testing (fit testing)
- Efficiency testing of HEPA filter assemblies
- Respirator design and development
- Filter design and development
- Aerosol laboratory research

### **Features and Benefits**

- Same photometer engine as used by NIOSH
- Filter-efficiency measurements to 99.999%
- Penetration versus particle size to 0.001%
- Fit factors to 100,000
- Indicates low airflow conditions
- Signal correlates with aerosol mass concentration
- Stable 30 mW laser light source
- Internal valve switches between upstream and downstream samples
- Automatic gain selection
- Analog and digital output
- Manual or remote control via RS-232
- Critical orifice controls sample airflow
- Plug-and-play compatibility with the original 8587 command language

## Background


In 1990, TSI® began developing an advanced-technology light scattering photometer to replace aging instruments incapable of measuring the high protection factors provided by newer gas mask designs. The result was the Laser Photometer 8587A, which is still in service for testing filter efficiency.

Moreover the photometer owners asked TSI® to develop a modern version of the Laser Photometer 8587 that retains data continuity with the original version. Without data continuity, vast amounts of legacy research would not be directly comparable to new research.

The model 8587A can also be used in HEPA filter scanning systems to measure the penetration efficiencies of large, high-efficiency filter assemblies.



**Flow Schematic Laser Photometer 8587A**

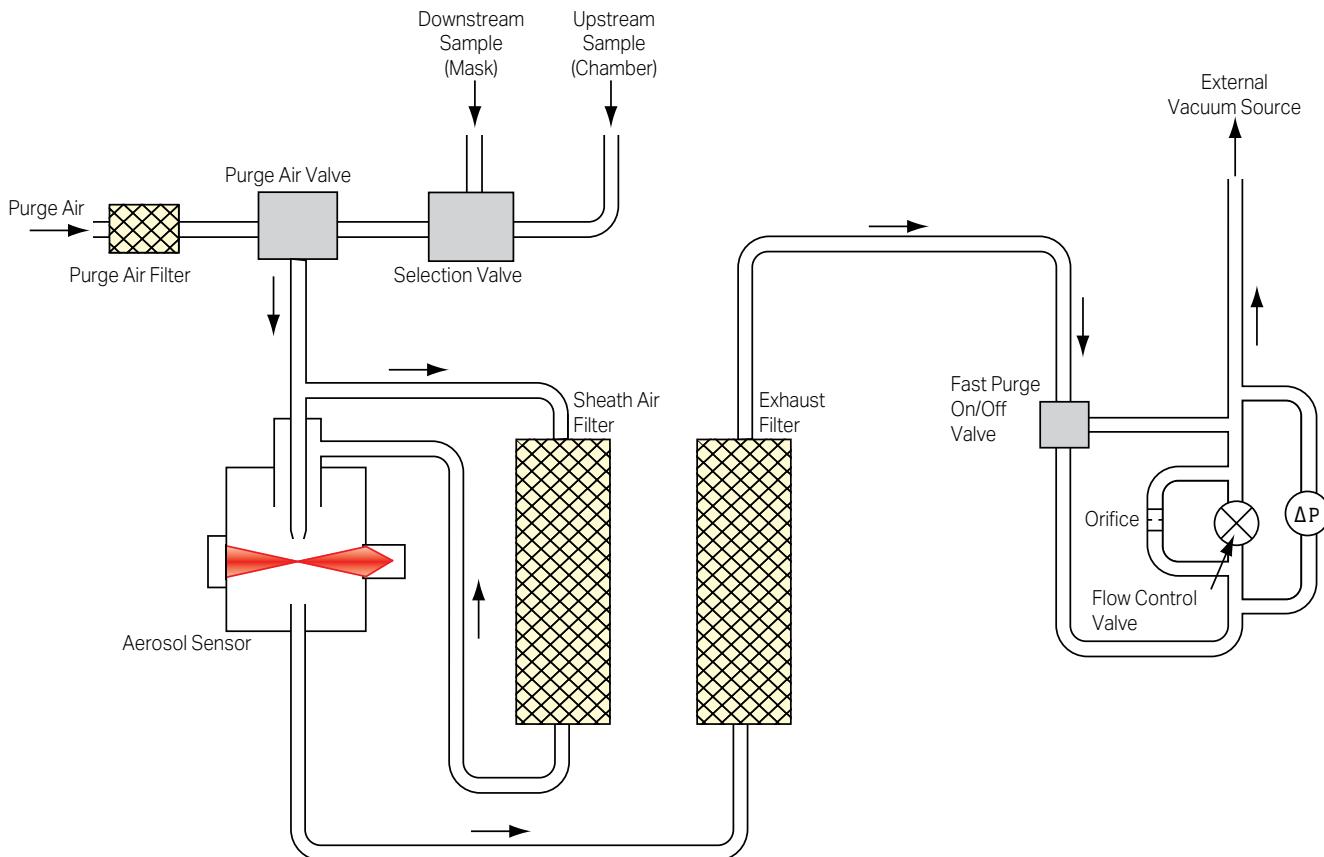

## Respirator Certification Testing

The Laser Photometer 8587A uses the same reliable, robust, time-proven photometer engine as the original model 8587 used by the US Army for gas mask development and by NIOSH for CBRN respirator certification testing. In fact, the 8587A is plug-and-play compatible with the original 8587. This means your laboratory can develop and test new respirator designs using the same measurement used for NIOSH certification testing.

## Operation

The model 8587A has a simple front panel keypad for manually switching between upstream sampling, purging and downstream sampling. It also has a digital photometer voltage display on the front panel, with the real-time analog voltage available via a back panel connector.

Most users will want to take advantage of the remote control features that allow precise test protocol control via an RS-232 interface. You can write your own software to control all aspects of testing, including sampling mode (i.e., upstream/purge/downstream), read voltage, reset voltage, query valve status, and to control all three valves individually.

## Low Maintenance


The optics are protected by filtered sheath air. Aerosols never come in contact with the lenses.

## Filter Testing

The model 8587A is perfect for testing the efficiency of particulate filters. In fact, the 8587A photometer engine is similar to the one used in the TSI® Automated Filter Tester 8130A currently employed by NIOSH for 42 CFR part 84 particulate filter certification. Integrated valves make switching between upstream, purge and downstream measurements simple using front panel or remote control.

## Laboratory Applications

The 8587A is useful for a variety of aerosol research applications. It is a basic photometer with switching valves added to accommodate easy aerosol concentration ratio measurements or mass correlations with a wide variety of aerosols.

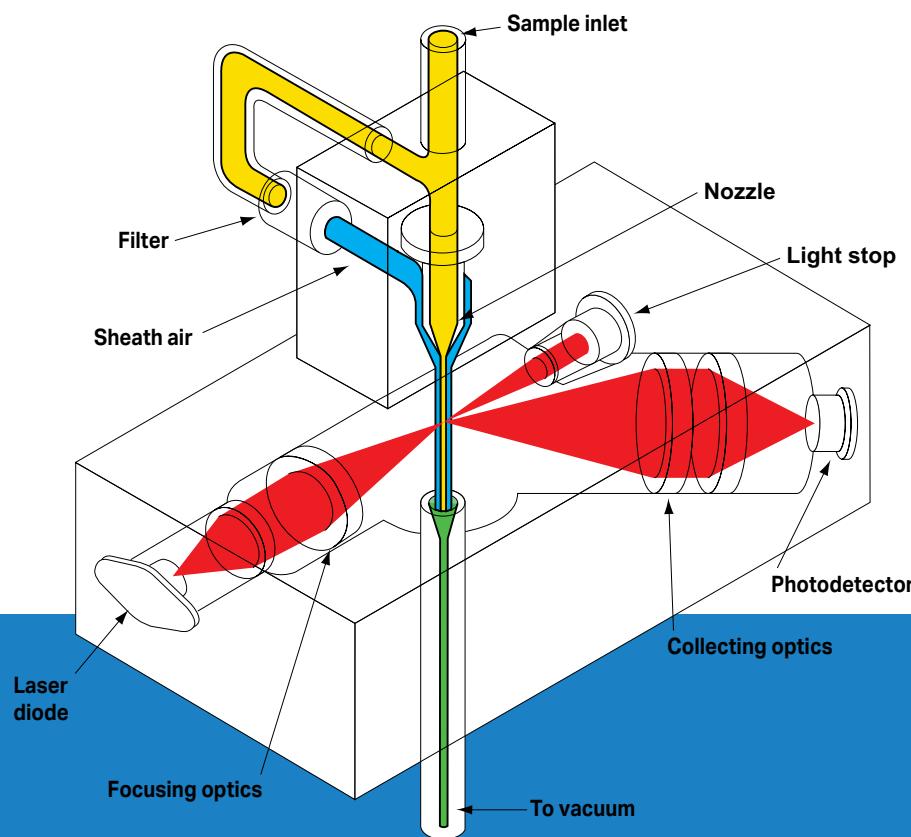

## Specifications

# Laser Photometer

## Model 8587A

### Photometer

Concentration Range	1.0 $\mu\text{g}/\text{m}^3$ to >200 $\text{mg}/\text{m}^3$ (0.000001 to 0.200 $\text{g}/\text{m}^3$ )
Dynamic Range	Fit factors to 100,000; filter efficiency to 99.999%
Gain Selection	Automatic

### Optics and Laser

Light Source	30 mW laser diode, 780 nm wavelength
Collection Angle	45 degrees
Lens Protection	Sheath air prevents aerosol from contacting optics

### Flow Rate

Sample	2.0 l/min (controlled with critical orifice)
Purge	Approx. 20 l/min (uncontrolled)

### Instrument Control

Manual	Front panel buttons
Remote	Computer control via RS-232

### Size (W x H x D)

15 cm x 25 cm x 33 cm (6.25 in. x 10 in. x 13 in.)

### Weight

6.4 kg (13.5 lb)

### Vacuum Pump\*

Sampling	2.0 l/min @ 55 kPa (8 psi) vacuum
Purging	20 l/min @ 0 kPa (ambient atmospheric pressure)

### Communications

Analog Output	0 to 5 VDC
RS-232	9-pin D-type (DB9F) connector; ASCII; 1200 bps or 115 Kbps (selectable), N, 8, 1

### Power

100 to 240 VAC, 50/60 Hz (auto-sensing),  
1.3 A, IEC 60320/C14 socket

### Front Panel

Display	16 character x 2 line LCD (backlit)
Control Buttons	Upstream, Purge, Downstream

### Back Panel

On/Off switch	
IEC 60320/C14 line cord socket	
Analog output female BNC connector	
RS-232 connector (DB9F)	
USB Type B female connector (factory use only)	
6.4 mm (0.25 in.) diameter upstream/downstream/vacuum ports	

### Software Provided

Documentation of 8587A ASCII command set (in Operation and Service Manual)

\*Purge flow is the determining factor in selecting a vacuum pump. Most pumps that provide the needed purge flow at atmospheric pressure will have no difficulty providing the needed flow during sampling.

Specifications are subject to change without notice. TSI and the TSI logo are trademarks of TSI Incorporated. Windows is a registered trademark of Microsoft Corporation. LabVIEW is a trademark of National Instruments Corporation.

### To Order

#### Laser Photometer 8587A

Specify	Description
8587A	Laser Photometer, 115/230 VAC, 60/50 Hz
3032	Vacuum pump for one photometer
3033	Vacuum pump for two to four photometers, Up-to 60 l/min, 115/230 VAC, 60/50 Hz
4140	Airflow meter to verify supply and sample airflows
1083636	Filter maintenance kit for 8587A



Knowledge Beyond Measure.

TSI Incorporated - Visit our website [www.tsi.com](http://www.tsi.com) for more information.

**USA** Tel: +1 800 874 2811  
**UK** Tel: +44 149 4 459200  
**France** Tel: +33 1 41 19 21 99  
**Germany** Tel: +49 241 523030

**India** Tel: +91 80 67877200  
**China** Tel: +86 10 8219 7688  
**Singapore** Tel: +65 6595 6388