Next Generation Impactor (NGI) Internal Filter

Installation Instructions

The Next Generation Impactor (NGI) Internal Filter consists of three components: Cup, Filter Support, and MOC Seal.

Additionally, 75-mm glass fiber filters are needed to complete the assembly (sold separately).

Cup	**Filter Support**	**MOC Seal**

To use the Internal Filter perform the following steps:

1. Remove the standard stage 8 (MOC) large cup from the NGI.

2. Place 75-mm glass fiber filter (sold separately) centered on top of the Filter Support. You may find it easier to already have it in the Internal Filter Cup.

3. Place MOC Seal over the top of filter, aligning the Filter Support tabs in the MOC Seal grooves.	
4. Filter Support will drop into the groove of Internal Filter Cup.	

5. Place the assembly in the standard stage 8 (MOC) NGI large cup well.

NOTICE
Aligning the laser markings on the Internal Filter Cup and MOC Seal, as shown, will provide maximum clearance and ensure proper closing without damage to the MOC or assembly.

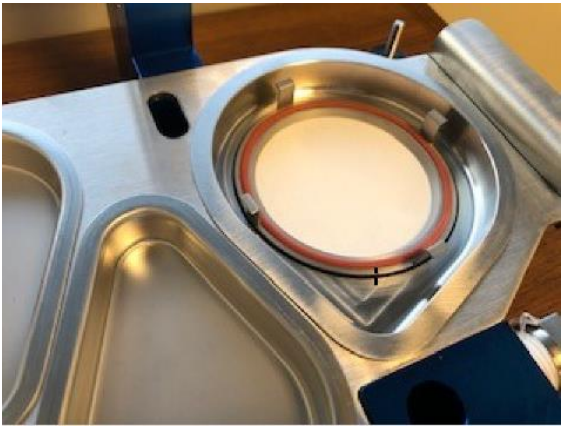

msp®
A DIVISION OF TSI

MSP - Visit our website **www.tsi.com/msp** for more information.

5910 Rice Creek Parkway, Suite 300
Shoreview, Minnesota
55126, U.S.A.
Tel: 651.287.8100

P/N 6013944-US Rev. B (2/23/2023) ©2023 TSI Incorporated Printed in U.S.A.